

**CLOROX**PRO<sup>®</sup>

# Product Reference Guide

Clorox<sup>®</sup> Turbo Pro<sup>™</sup>  
*Disinfectant Cleaner*

*For use with TurboPro<sup>™</sup> devices*



# Clorox® Turbo Pro™ Disinfectant Cleaner

- ▶ **Disinfectant cleaner that cleans, disinfects and deodorizes hard, nonporous surfaces**
- ▶ **Kills 51 pathogens, including the COVID-19 causing virus, cold and flu viruses, MRSA and norovirus in 2 minutes or less**
- ▶ **Sanitizes soft surfaces in 2 min**
- ▶ **Tested for use with Clorox® TurboPro™ handheld electrostatic sprayer (item #29561) and other electrostatic devices**



Clorox® Turbo Pro™  
Disinfectant Cleaner  
121 fl. oz.  
Item No.: 60091

At a Glance Clorox® Anywhere® Daily Disinfectant & Sanitizer	
<b>EPA Registration No</b>	67619-38 (Puff)
<b>Product Type</b>	Ready to Use For use with TurboPro™ HandHeld Electrostatic Sprayer and other electrostatic sprayer devices
<b>Cleaning Chemical Type</b>	<ul style="list-style-type: none"> <li>▶ 1-step cleaner disinfectant (hard surfaces)</li> <li>▶ Sanitizer (hard/soft surfaces)</li> <li>▶ Deodorizer (hard/soft surfaces)</li> <li>▶ Inhibits mold growth for 7 days (hard surfaces)</li> </ul>
<b>Active Ingredient</b>	Quat (0.3%)
<b>pH</b>	11.9
<b>Odor</b>	None
<b>Shelf Life</b>	3 years from the manufactured date on label
<b>Toxicity Signal Word</b>	Caution   <a href="#">SDS link</a>
<b>HMIS Rating</b>	1-0-0-X
<b>PPE Required</b>	Eye protection and protective gloves are recommended when using through the TurboPro™ Handheld Electrostatic Sprayer

\* *Staphylococcus aureus* [(Staph)], *Klebsiella pneumonia* [(Kleb)]

# Disinfection Efficacy Claims

Disinfection	Contact Time
<b>BACTERIA</b>	
<i>Bordetella bronchiseptica</i>	2 min
<i>Bordetella pertussis</i>	2 min
<i>Campylobacter jejuni</i>	2 min
Community associated methicillin-resistant <i>Staphylococcus aureus</i>	2 min
<i>Enterococcus faecalis</i>	2 min
<i>Escherichia coli</i> O157:H7	2 min
Extended Spectrum Beta-Lactamase (ESBL) producing <i>Escherichia coli</i>	2 min
<i>Klebsiella aerogenes</i> tested as <i>Enterobacter aerogenes</i>	2 min
<i>Klebsiella pneumoniae</i>	2 min
<i>Legionella pneumophila</i>	2 min
<i>Listeria monocytogenes</i>	2 min
Methicillin-Resistant <i>Staphylococcus aureus</i> (MRSA)	2 min
Multi-drug Resistant (MDR) <i>Acinetobacter Baumannii</i>	2 min
Multi-drug Resistant <i>Streptococcus pneumoniae</i>	2 min
<i>Mycoplasma gallisepticum</i>	2 min
<i>Mycoplasma orale</i>	2 min
New Delhi Metallo-Beta Lactamase (NDM-1) producing Carbapenem Resistant <i>Klebsiella pneumoniae</i>	2 min
<i>Pseudomonas aeruginosa</i>	2 min
<i>Salmonella enterica</i>	2 min
<i>Staphylococcus aureus</i>	2 min
<i>Staphylococcus epidermidis</i>	2 min
<i>Streptococcus pyogenes</i>	2 min
Vancomycin-Resistant <i>Enterococcus faecium</i>	2 min
<b>FUNGI</b>	
<i>Microsporum canis</i>	2 min
<i>Trichophyton interdigitale</i>	10 min
<b>VIRUSES</b>	
Avian Influenza Virus (H5N1)	30 sec
Bovine Viral Diarrhea Virus as Hepatitis C Virus	1 min
Canine Coronavirus	2 min
Canine Distemper Virus	5 min
Canine Influenza Virus (H3N8)	2 min
Cytomegalovirus	2 min

Disinfection	Contact Time
<b>VIRUSES</b>	
Duck Hepatitis B Virus (surrogate for HBV)	1 min
Feline rhinotracheitis Virus	2 min
Herpes Simplex Virus Type 1	2 min
Human Coronavirus	2 min
Human Immunodeficiency Virus Type 1 (HIV-1)	30 sec
Influenza A Virus	2 min
Measles Virus	2 min
Mumps Virus	2 min
Respiratory Syncytial Virus (RSV)	2 min
Rubella Virus	2 min
SARS-CoV-2	2 min
Adenovirus Type 2	2 min
Human Rotavirus	1 min
Canine Parvovirus Type 2b	2 min
Coxsackievirus Type B3	5 min
Feline calicivirus as surrogate for Norovirus	2 min
Feline panleukopenia virus	2 min
Poliovirus	5 min
Rhinovirus Type 14	2 min
Rhinovirus Type 39	2 min
<b>Sanitization (Hard, Nonporous Surfaces)</b>	
<b>BACTERIA</b>	
<i>Staphylococcus aureus</i>	5 sec
<i>Klebsiella pneumoniae</i>	5 sec
<b>Sanitization (Soft Surface)</b>	
<b>BACTERIA</b>	
<i>Klebsiella aerogenes</i> tested as <i>Enterobacter aerogenes</i>	2 min
<i>Staphylococcus aureus</i>	2 min
<b>Fungistat</b>	
<b>FUNGUS</b>	
<i>Aspergillus niger</i>	7 days



# Directions for Use TurboPro™ Handheld Electrostatic Sprayer and other electrostatic devices

## Step 1: Preparation



1. Gather supplies




2. Wash hands with soap and water



3. Put on PPE required by your facility<sup>1</sup>


1. Eye protection and gloves are recommended. We recommend following your facility's PPE policy




4. Make sure the area is well ventilated



5. Close off area




6. Make sure battery is charged. Be sure switch is in the locked or OFF position before inserting battery pack




7. Align tank grooves into slide rail and lower sprayer onto the tank



8. Listen for a click



9. Rotate collar to locked position

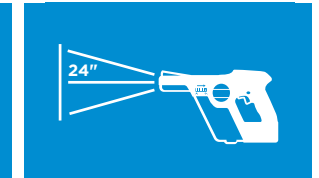


10. Pull the trigger and spray surface from 2-3 feet away

## Step 2: Application


To disinfect or sanitize hard, nonporous surfaces in general areas



1. Clean visible soil (spot clean)

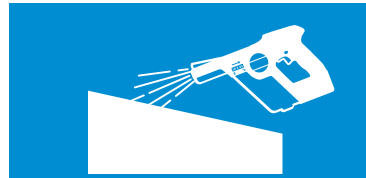


2. Spray in a slow, S-shaped motion from high to low, 2-3 ft. from surface

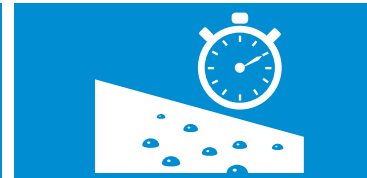

3. Surface needs to stay wet for the contact time<sup>2</sup>

2. Contact times range from 30 sec-10 min., depending on the pathogen. See the Disinfection Efficacy Claims page for exact contact time

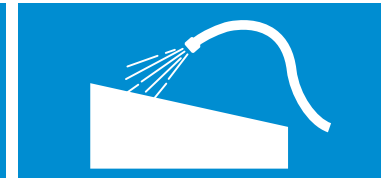


4. Rinse or wipe clean. Allow to air dry



# Directions for Use TurboPro™ Handheld Electrostatic Sprayer and other electrostatic devices

## To disinfect or sanitize hard, nonporous surfaces in food processing/food service premises

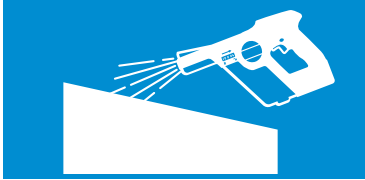

**1.** Spray in a slow, S-shaped motion from high to low, 2-3 ft from surface




**2.** Surface needs to stay wet for the contact time<sup>2</sup>

2. Contact times range from 30 sec-10 min., depending on the pathogen. See the Disinfection Efficacy Claims page for exact contact time



**3.** Rinse or wipe clean. Allow to air dry

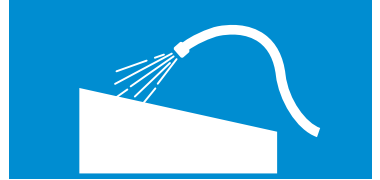


**4.** Thoroughly rinse all food contact surfaces with potable water or wipe with clean damp cloth

## To sanitize soft surfaces



**1.** Spray in a slow, S-shaped motion from high to low, 2-3 ft from surface. Do not oversaturate

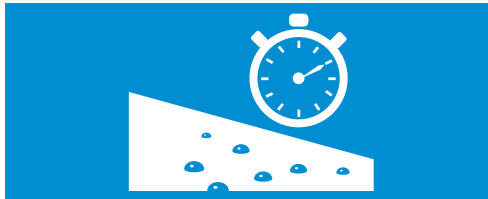


**2.** Surface needs to stay wet for the contact time of 2 min




**3.** Allow to air dry

## To control mold and mildew on hard, nonporous surfaces

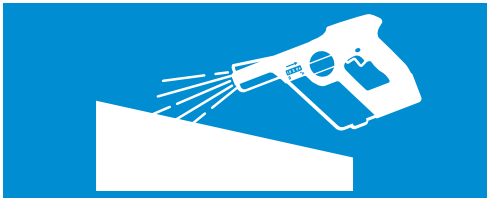

**1.** Spray in a slow, S-shaped motion from high to low, 2-3 ft. from surface

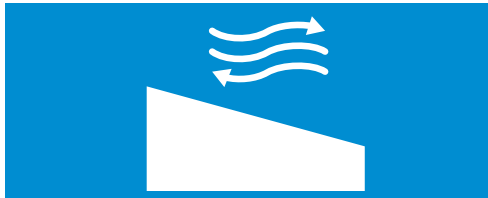

**2.** Allow to air dry




**3.** Repeat weekly



# Directions for Use TurboPro™ Handheld Electrostatic Sprayer and other electrostatic devices


## Step 3: Wrap Up

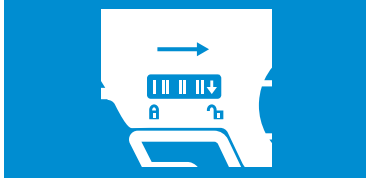


**1.** Rotate collar to unlock position




**2.** Pull locking ring to remove

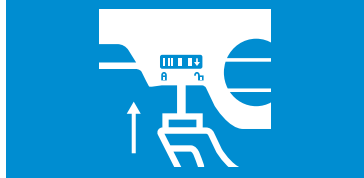


**3.** Lift sprayer unit off the tank

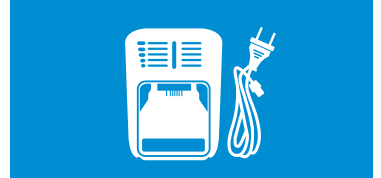

**4.** Disconnect battery pack from cordless sprayer in the locked or OFF position

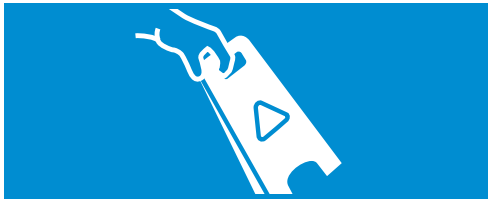

**5.** Reopen the area

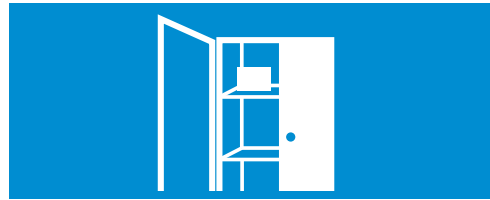

**6.** Store idle cordless sprayer out of reach of children. Ensure that all individuals are trained to use the device before handling



**7.** Store battery pack away from other metal objects



# Common Applications



## Classrooms — Disinfect

- ▶ Desks
- ▶ Chairs
- ▶ Sinks
- ▶ Water fountain exteriors



## Conference Rooms — Disinfect

- ▶ Tables
- ▶ Cords
- ▶ Computers
- ▶ Keyboards



## Offices — Disinfect

- ▶ Cabinets
- ▶ Workstations
- ▶ Electronics\*



## School Buses — Disinfect

- ▶ Buttons
- ▶ Rails
- ▶ Steering wheels
- ▶ Seats



## Elevators/Stairwells — Disinfect

- ▶ Buttons
- ▶ Walls
- ▶ Handrails
- ▶ Floors



## Dorms and hotel rooms — Disinfect

- ▶ Plastic or vinyl mattress covers
- ▶ Coated mattresses
- ▶ Bathroom surfaces
- ▶ Bedside tables


\* For any use site that includes electronic components, please refer to manufacturers' instructions before use

# Surface Compatibility

This product is safe for use on these surface materials.\*



Acrylic



ABS




Aluminum



Chrome



Corian®



Formica®



Glass




Glazed Ceramic



Glazed Porcelain



Sealed Stone



Laminate




Plastic



Stainless Steel



PVC



Sealed Fiberglass



Silicone Rubber



Vinyl

Not recommended for use on paper and untreated/unpainted wood

## PRO TIP

If you're unsure about compatibility with a certain surface, contact the manufacturer or test it on the surface in an inconspicuous area prior to using it more widely. To prevent residue build-up and further reduce the risk of potential surface damage, wipe periodically with a clean damp cloth to remove residue and excess disinfectant.

\* Compatibility with equipment and surfaces, including electronic surfaces, will vary based on the components and material coatings. Check with the manufacturer for guidance on approved products for disinfection. Corian® is a registered trademark of E. I. du Pont de Nemours and Company. Formica® is a registered trademark of The Diller Corporation.





# Product Storage & Disposal

## STORAGE


### Do's



Secure bottle (container tightly closed)



Store in a cool, dry, well-ventilated place

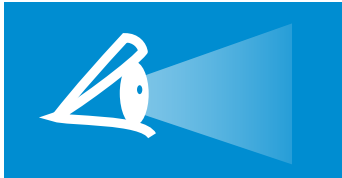

Store at or below eye level for safety precaution


### Don'ts



Do not freeze



Do not store in a location accessible to children

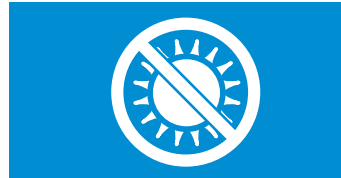


Keep out of direct sunlight

## DISPOSAL

### Chemical

#### Do's

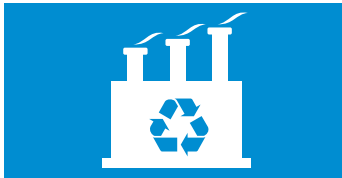

Dispose of at an approved waste disposal facility



Contact your local environmental, health or solid waste agency for proper disposal of the chemical

#### Don'ts



Pour it down the drain or toilet, on the ground, into storm sewers. Do not contaminate water, food or feed by disposal.



Dispose with regular trash

### Container

#### Do's



Recycle plastic container

#### Don'ts



Reuse or refill plastic container

**CLOROXPRO**

# Product Safety

**Precaution for safe handling:** Handle in accordance with good industrial hygiene and safety practices

**Most important symptoms and effects:** May cause slight eye irritation

## First Aid:



**Eye contact:** may cause slight irritation

- ▶ Hold eye open and rinse gently with water for 15-20 min.
- ▶ If present, remove contact lenses after the first 5 min. of rinsing, then continue rinsing eye



**Skin contact:** not irritating

- ▶ Wash skin with soap and water



**Inhalation:** may cause minor irritation to respiratory tract

- ▶ Move to a place with fresh air



**Ingestion:** may cause slight irritation to mucous membranes and gastrointestinal tract

- ▶ Rinse mouth and drink plenty of water

If irritation or other symptoms such as breathing problems persist call a doctor.

### National Fire Protection Association (NFPA) Ratings:

Health Hazard: 1  
Flammability: 0  
Instability: 0  
Physical and Chemical Hazards: None

### Hazardous Material Identification System (HMIS) Ratings:

Health Hazard: 1  
Flammability: 0  
Physical Hazard: 0  
Personal Protection: None

**Questions:** Call (800) 492-9729

**SDS:** Much of this information and more can be found on the SDS. Make sure to have a printed product SDS within 10 min of travel time, so it is easily accessible. Click [here](#) for a link to the product SDS.

